



Disponible en ligne sur

ScienceDirect
www.sciencedirect.com

Elsevier Masson France

EM|consulte
www.em-consulte.com



ORIGINAL ARTICLE

Evaluation and comparison of basic gestures in ex vivo laparoscopic surgery using a robotic instrument and traditional laparoscopic instruments



Évaluation et comparaison ex-vivo de gestes de base en chirurgie laparoscopique réalisés à l'aide d'un instrument robotisé ou d'instruments de laparoscopie classique

F.-X. Madec^{a,*}, C. Dariane^b, J.-N. Cornu^c

^a Service d'urologie, hôpital Foch, université de Versailles - Saint-Quentin-en-Yvelines, 40, rue de Worth, 92150 Suresnes, France

^b Service d'urologie, hôpital européen Georges-Pompidou, 20, rue Leblanc, 75015 Paris, France

^c Service d'Urologie, CHU de Rouen Charles-Nicolle, 1, rue de Germont, 76000 Rouen, France

Received 29 April 2018; accepted 28 November 2019

Available online 27 December 2019

KEYWORDS

Pelvitainer;
Laparoscopy;
Robotic instrument;
Dry lab

Summary

Background. — The robotic Dextérité Surgical™ arm (DEX) is an instrument used in laparoscopy that provides 6 degrees of freedom and 360 degrees of rotation with a needle holder and scissors. To evaluate the benefits this instrument offers, we asked novice surgeons to use DEX and a conventional laparoscopic instrument on a pelvitainer and compared the results.

Methods. — The participants were asked to perform two exercises with DEX and then with a conventional laparoscopic instrument on a pelvitainer that contained a synthetic reproduction of a male pelvis. For the stitching exercise, the distance from the marked points and any tears caused were analyzed. For the cutting, the participants were judged by how well they respected the marked extremities, the form and the amount of “hacking” observed on a multi-criteria scale. The amount of time required to carry out the exercises was recorded.

* Corresponding author.

E-mail address: madecfx@hotmail.com (F.-X. Madec).

Results. — All twelve urology interns all succeeded in using DEX. Of the 36 stitches, seven were giving a failing grade (19.4%) when using the conventional laparoscopic needle holder and one (0.3%) was recorded when using DEX. All of the criteria (entry and exit points, tears and duration) for the results obtained were better when using DEX compared to the classic laparoscopic tool. This difference was statistically significant for horizontal stitches and tearing. Concerning the cuts made, the global score obtained, following a multi-criteria scale, favored the use of DEX for 10 out of 12 candidates (83.3%) with an average score of +2.6 (± 2.1). No significant difference was recorded for the duration of each exercise.

Conclusion. — It does not take novice operators long to understand how to use DEX. It enables precise stitching and reduces tearing while improving the quality of cuts compared to conventional laparoscopic instruments, all without slowing the user down.

Level of evidence. — 4.

© 2019 Elsevier Masson SAS. All rights reserved.

MOTS CLÉS

Pelvitainer ;
Laparoscopie ;
Instrument robotisé ;
Simulation

Résumé

Introduction. — Le bras robotisé Dextérité Surgical™ (DEX) est un instrument utilisé en laparoscopie permettant 6 degrés de liberté et une rotation de 360 degrés avec un porte-aiguille ou un ciseau. Pour évaluer les bénéfices de cet instrument, nous avons comparé l'utilisation de DEX avec les instruments de laparoscopie conventionnelle chez des chirurgiens débutant sur pelvitainer.

Méthodes. — Les participants devaient réaliser 2 exercices (passage d'aiguille et découpe) avec DEX puis des instruments de laparoscopie sur des pelvitainers contenant une reproduction synthétique de pelvis masculin au fond duquel était fixée une lame en silicone. Pour le passage d'aiguille, l'écart entre les points d'entrée et les points de sortie prévus ainsi que les déchirures étaient analysés. Pour la découpe, le respect des extrémités, la forme ainsi que l'aspect haché étaient évalués sur une échelle multicritères. Le temps de réalisation des exercices était chronométré.

Résultats. — Les douze internes d'urologie ont réussi à utiliser DEX. Sur les 36 passages de points, sept échecs (19,4 %) ont été constatés avec le porte-aiguille de laparoscopie et 1 avec DEX (0,3 %). Sur tous les critères (points d'entrée, de sortie, déchirure, temps) les résultats obtenus apparaissaient meilleurs avec DEX par rapport à la laparoscopie classique. Cette différence était statistiquement significative pour le passage des points horizontaux, et les déchirures. Pour la découpe, le score global obtenu selon l'échelle multicritères favorisait DEX pour 10 candidats sur 12 (83,3 %) avec un score de +2,6 ($\pm 2,1$). Il n'y avait pas de différence significative pour la durée de réalisation des exercices entre les 2 instruments.

Conclusions. — DEX est manipulable rapidement par des opérateurs peu expérimentés. Il permet un passage d'aiguille plus précis avec moins de déchirure et améliore la découpe par rapport à la laparoscopie conventionnelle, sans ralentir l'exécution des gestes.

Niveau de preuve. — 4.

© 2019 Elsevier Masson SAS. Tous droits réservés.

Introduction

Laparoscopic surgical approaches are frequently employed in urological surgery. The main benefits of this minimally-invasive surgery rely on the reduction of pain, size of incisions, days of hospitalization and recovery times [1]. The major difficulty of this technique is related to the fact that conventional laparoscopic instruments are not articulated and rely on the abdominal wall to serve as a pivot-point, which reduces the degree of freedom [2]. Robotization of the instruments allows to correct this problem

and realize deep and complex laparoscopic gestures, such as cutting with the scissors and stitching with a needle, much easier to perform by granting trocars with 360° of rotation. The robotic arm from DEXTERITE Surgical™ (Dexterite Surgical Inc based in Annecy, France) has been used for general, urologic, and gynecologic surgeries in France since 2010. The distal extremities (the needle holder and the scissors) are free to move in three planes and have 6 degrees of freedom as well as unlimited rotation. In addition, thanks to the ergonomic and articulated handle, the instrument preserves haptic return, or force feedback (Fig. 1).



Figure 1. Dextérité Surgical™ robotized instrument (needle holder and scissors).

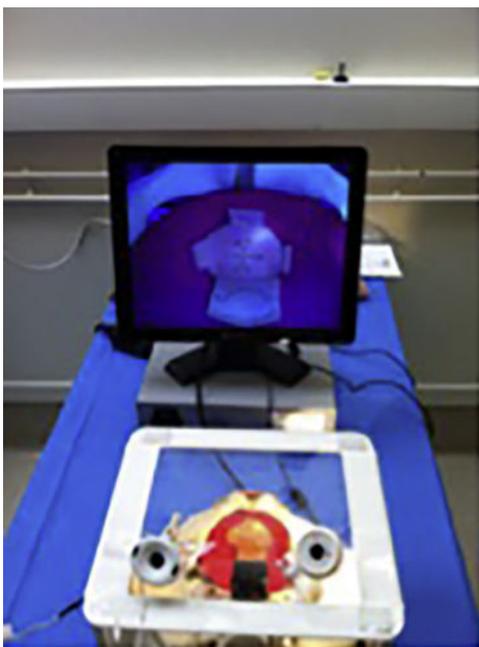


Figure 2. Pelvitainer model used for both exercises (stitching and cutting).

In order to evaluate the benefits of this instrument when using pelvitainer, we studied the experiments of novice operators using the Dextérité (DEX) arm and compared them to their experiments using conventional laparoscopic instruments.

Methods

Study design

This study was conducted in 2014 at the Assistance publique des Hôpitaux de Paris (AP-HP) – School of Surgery Fer à Moulin.

Six pelvitainers were used. Each pelvitainer was equipped with a synthetic reproduction of the male pelvic skeleton on which a thin layer of foam was fixed to represent the muscles of the pelvic floor. The pelvitainers thus simulated the spatial constraints involved in urologic operations such as radical prostatectomies. Towards the rear of each model we fixed a silicone plate to enable the operators to conduct their exercises in the frontal plane (Fig. 2).

This cross-over comparative study required each participant to carry out 2 exercises, using their dominant hand to successively manipulate the Dextérité (DEX) robotic arm

followed by a standard laparoscopic instrument (the needle holder and 5 mm scissors from Karl Storz endoscope, Inc).

The endoscope had a 0° laparoscopic optic and its position, as well as that of the model, was standardized in the pelvitainer. Participants held fenestrated laparoscopic surgical pliers in their non-dominant hand.

DEX is a robotic co-manipulation instrument which contains a console and a 10mm-diameter handle, equipped with micro-motors, to which the surgical instrument (the needle holder or scissors) can be connected.

Participants

All participants were urologists residents, all belonging to the French Association of Urologists in Training (AFUF). Students in their first two years of residency were considered as “beginners”, because they were still in general surgery. The older residents were considered as « experienced » as they were registered for the complementary specialized diploma in urological surgery.

Task and evaluation

The session began with 20 minutes of instructions to cover the objectives of the study and the utilization of the DEX tool. Then, the exercises were carried out without giving the operators any opportunity to practice using the pelvitainers.

Two exercises were evaluated: the stitching with the needle and the cutting. For the first exercise, a silicone block was used with landmarks on its surface. Each participant was asked to pass the needle in and out of the silicone following each of the landmarks three times. The vertical crossing went from the point 1A to the point 1B (from bottom to top), the horizontal crossing from the point 2A to the point 2B (from left to right) and the oblique crossing from the point 3A to the point 3B. For each vertical, horizontal and oblique crossing, the distance was measured in millimeters between the entry points (1A, 2A and 3A) and the exit points (1B, 2B and 3B). The time spent for each participant to place the needle in the instrument and to pass the stitches was recorded in seconds. Any rips in the silicone caused by the needle were evaluated, on a scale of 0 to 3, depending on the visible constraints. Failure was evaluated if there were more than 10 mm between the landmarks and the needle’s actual entry points or if it took the participant more than 20 minutes to begin stitching.

For the second exercise, participants were asked to cut along a marked line in the form of an omega (Fig. 3). The quality of the cut was evaluated following a number of different criteria and the time spent to the participant to carry out the task was recorded. The three criteria were as followed: respecting the 2 extremities that represented the beginning and the end of the omega’s circle, the way they followed the rounded line and the amount of “hacking” along the whole line. Each parameter was evaluated following the difference between the results obtained using each tool: we added +1, +2 or +3 points when the result was obtained better with the DEX tool, and we subtracted –1, –2 or –3 points if the use of the classic laparoscopic tool permitted a better result. A score of 0 was attributed if the results using each tool were equivalent. An overall positive

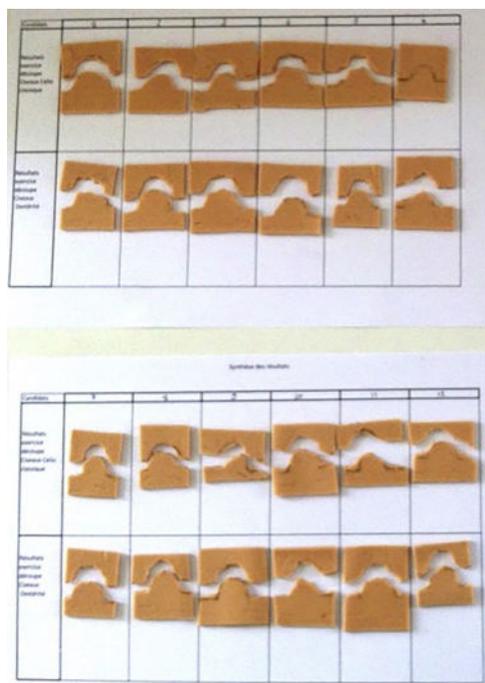


Figure 3. Comparison of the 12 residents' "Omega" cut pattern exercises using conventional laparoscopic instruments (upper line) and DEX (lower line).

score is in favour of DEX tool and a negative for laparoscopic tool.

The exercises were evaluated anonymously, after-the-fact and outside of context by 2 senior surgeons, experts in laparoscopy.

A survey to evaluate the ergonomics, on a scale of 0 to 10, was sent to each participant the day of the study. It included an evaluation of the postural comfort and the simplicity of use of DEX.

Statistical analysis

Data are expressed as percentage with [standard deviation]. The average scores for each participant were calculated and compared with the Mann–Whitney test. A sensitivity analysis using a student test was performed to compare beginners and experienced residents for the second exercise (cutting exercise) using DEX or laparoscopic instrument.

Statistical analyses were done using the Prism 7 software. A *P* value inferior to 0.05 was considered as statistically significant.

Results

Twelve urology residents (9 men and 3 women – 5 in their 3rd semester, 5 in their 5th semester and 2 in their 7th semester). Five participants were beginners and 7 were experienced. The residents had spent 2 ± 0.95 rotations in a urological department and 1.6 ± 0.5 rotations in visceral surgery, $P < 0.05$. All participants had at least made 1 pelvi-trainer session and assisted routinely in the operative room for laparoscopic surgery.

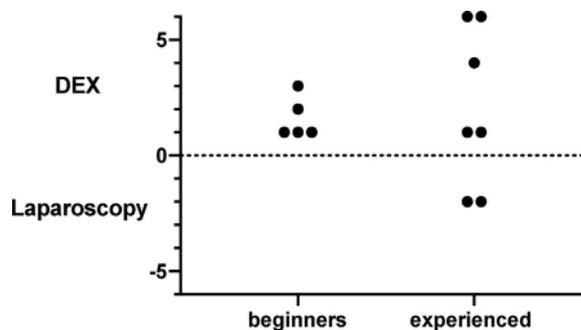


Figure 4. Sensitivity analyse of the cutting score between beginners and experienced residents. An overall positive score is in favour of DEX tool and a negative for laparoscopic tool. In the experienced group, the global cutting score was $2 (\pm 3.4)$ and $1.8 (\pm 0.9)$ in the beginners group without any significant difference ($P > 0.05$).

All of the participants were able to use DEX successfully, without additional training, after the 20 minutes included in the exam.

For the first exercise, a total of 36 needle passes with each instrument were analysed. Seven out of 36 needle passes (19.4%) received failure grades when using the laparoscopic needle holder and one (0.3%) when using DEX. For all of the criteria (entry and exit points, rips and time) the results obtained were better when using DEX compared to the classic laparoscopic tool [Table 1]. This difference was statistically significant regarding the horizontal needle passes, with a difference of $2.7 \text{ mm} \pm 1.6$ in the classic tool group comparing to $0.4 \text{ mm} \pm 0.6$ in the DEX group ($P = 0.002$). The rips were significantly reduced in the vertical ($P = 0.04$) and horizontal ($P = 0.003$) crossings. There were no significant differences for either group of tools in the time spent for each participant to set up the needle and complete their stitching.

For the second exercise, the global cutting score obtained following the multi-criteria scale was in favor of the DEX tool for 10 of the 12 participants (83.3%). In this group, the average score was $+2.6 (\pm 2.1)$. The remaining two participants scored negative points $-2 (\pm 0)$ in favor of the classic tool. One participant was able to perform the cut using DEX but could not carry out the same task with the classic tool.

The participants obtained positive scores when using DEX when it came to respecting the 2 extremities of the omega's circle, the round contour and the hacking aspect: $+1.1 (\pm 0.9)$; $+0.5 (\pm 1.2)$; $+0.3 (\pm 1.3)$ respectively.

The times recorded for the cutting exercise were similar for the two groups: 128 seconds (± 76) for DEX and 70 (± 17) for the laparoscopic arm. The average time spent to complete the cutting exercise was longer when using DEX ($P = 0.052$). A sensitivity analyse was performed to compare the quality of cutting between beginners and experienced residents. The analyse didn't find any significant difference between both groups (Fig. 4), with a global cutting score of $2 (\pm 3.4)$ in the experienced groupe and $1.8 (\pm 0.9)$ in the beginners group ($P > 0.05$). The results were still in favor of DEX in both groups regardless of resident level.

Among the 12 residents, 7 (58.3%) responded to the ergonomic survey. All of the participants noticed that the postural comfort was satisfactory when using the DEX

Table 1 Comparison of average results of needle-passing exercises using conventional laparoscopy and DEX.

| Operating parameters | Conventional laparoscopy | DEX | P |
|--|--------------------------|--------------|-------|
| Gap from entry point (1A) for stitch 1 (mm) | 0.77 ± 1.0 | 0.66 ± 0.8 | 0.94 |
| Gap from exit point (1B) for stitch 1 (mm) | 4.0 ± 2.5 | 2.9 ± 1.8 | 0.44 |
| Gap from entry point (2A) for stitch 2 (mm) | 2.7 ± 1.6 | 0.4 ± 0.6 | 0.002 |
| Gap from exit point (2B) for stitch 2 (mm) | 7.0 ± 4.7 | 3.3 ± 2.1 | 0.1 |
| Gap from entry point (3A) for stitch 3 (mm) | 2.2 ± 2.2 | 0.75 ± 0.78 | 0.07 |
| Gap from exit point (3B) for stitch 3 (mm) | 3.1 ± 2.2 | 2.9 ± 1.6 | 0.87 |
| Timing for needle placement on the instrument, before stitch 1 (s) | 93.0 ± 58.0 | 63.0 ± 40.0 | 0.26 |
| Timing for needle placement on the instrument, before stitch 2 (s) | 162.0 ± 79.0 | 125.0 ± 85.0 | 0.33 |
| Timing for needle placement on the instrument, before stitch 3 (s) | 86.0 ± 83.0 | 81.0 ± 64.0 | 1.0 |
| Timing to pass stitch 1 (s) | 68.0 ± 88.0 | 47.0 ± 19.0 | 0.79 |
| Timing to pass stitch 2 (s) | 55.0 ± 56.0 | 52.0 ± 45.0 | 0.64 |
| Timing to pass stitch 3 (s) | 80.0 ± 99.0 | 37.0 ± 24.0 | 0.46 |
| Rip score for stitch 1 (scale of 0 to 3) | 1.1 ± 1.1 | 0.25 ± 0.45 | 0.04 |
| Rip score for stitch 2 (scale of 0 to 3) | 1.75 ± 0.9 | 0.5 ± 0.5 | 0.003 |
| Rip score for stitch 3 (scale of 0 to 3) | 0.9 ± 0.9 | 0.5 ± 0.5 | 0.29 |

scissors and needle holder (average score: 8.5 ± 1.6). The question concerning the simplicity of use scored $6.9 (\pm 1.5)$.

Discussion

During this study, using DEX, without any prior training, improved novice operator's scores when cutting and suturing compared to the use of conventional laparoscopic instruments.

The precision when passing the needle, as well as the reduction in tearing was statistically improved when using DEX compared to the conventional tool.

As reported by Bensignor et al. [3] using the JAIMY™ robotic needle holder, developed in collaboration with the Endocontrol Company (Grenoble, France), our results showed that DEX improved the effectiveness and quality of sutures obtained with a greater degree of freedom which helps the user to control the needle's trajectory [4].

The overall aspect of the cuts was improved in 83.4% of the participants when they used DEX. This superiority was true for all three evaluation parameters defined. To our knowledge, this important advantage, particularly necessary in excision surgery, had never been associated with the use of co-manipulation robotic instruments.

Using DEX does not seem to prove difficult since the participants were able to use it effectively after only 20 minutes of theoretic training. This compares favorably to the learning curve required for another articulated instrument with a needle holder difficult to use for beginners operators. [5]. Because the participants using DEX did not receive prior training, the results were not over-valued by repeating the gestures.

The time spent to set up the needle and the duration of the cutting exercise were similar between the two instruments, showing that the use of DEX can be intuitive and benefits from a fast learning curve. DEX limits the physical constraints responsible for musculoskeletal discomfort habitually reported when using conventional laparoscopic

instruments [6]. This observation was confirmed by the participants.

To date, two types of robotic instruments have been developed in surgery: those with remote-handling capabilities represented by the surgical systems from the DA Vinci Intuitive Surgical Inc (CA, USA), and co-manipulation systems similar to DEX. The training and time spent to suture using the remote surgical techniques seems faster than with conventional laparoscopic instruments [7]. However, the elevated cost of remote-handling surgeries and the absence of benefits provided by laparoscopic tools challenge the idea to generalize the use of this technique [8]. Some experts in minimally-invasive surgery agree that the benefits provided by remote-handling tools are not required for the duration of an operation, but only during some precise steps of the procedure [9]. Robotic co-manipulation arms, such as DEX, are less expensive and offer continuous benefits, and then represent a therapeutic alternative that improves the surgeon's performance while providing a more balanced benefits-to-cost ratio. Another advantage of robotic co-manipulation instruments compared to remote-surgery is the opportunity for the surgeon to remain close to the patient, in sterile conditions, in case a conversion is required. The instruments also preserve the haptic return which is lost in robotic remote surgery [10].

This study was conducted using operators beginners to the laparoscopic instruments. This allowed us to limit any bias towards the habitual use of conventional tools which would have inflated the results. In addition, the use of a synthetic, skeletal pelvic model enabled us to reproduce spatial constraints experienced in real, clinical situations in urologic surgery.

Because the tasks were performed using the pelvitrainer and the pool of participants was small, these first results require confirmation using cadavers or animals so that the different exercises representing urologic interventions can be compared. It would also be equally interesting to carry out a study dedicated to the ergonomic benefits of DEX and to clearly define its required learning curve.

Conclusion

Using DEX is possible for novice operators after only a short training period. It improves the needle passing techniques while reducing tearing, and improves the quality of cuts compared to conventional laparoscopic instruments, without slowing the operator down.

Acknowledgements

The authors thank the French Association of Urologists in Training (AFUF) for helping us recruit residents for the study and the management at the École de chirurgie du fer à Moulin, and their team, for allowing us to carry out this study.

Disclosure of interest

The authors declare that they have no competing interest.

References

- [1] Buia A, Stockhausen F, Hanisch H. Laparoscopic surgery: a qualified systematic review. *World J Methodol* 2015;5:238–54.
- [2] Okken LM, Chmarra MK, Hiemstra E, Jansen FW, Dankelman J. Assessment of joystick and wrist control in hand-held articulated laparoscopic prototypes. *Surg Endosc* 2012;26:1977–85.
- [3] Bensignor T, Morel G, Reversat D, Fuks D, Gayet B. Evaluation of the effect of a laparoscopic robotized needle holder on ergonomics and skills. *Surg Endosc* 2016;30:446–54.
- [4] Waseda M, Inaki N, Torres Bermudez JR, Manukyan G, Gacek IA, Schurr MO, et al. Precision in stitches: radius surgical system. *Surg Endosc* 2007;21:2056–62.
- [5] Martinec DV, Gatta P, Zheng B, Denk PM, Swanström LL. The trade-off between flexibility and maneuverability: task performance with articulating laparoscopic instruments. *Surg Endosc* 2009;23:2697–701.
- [6] Dalager T, Sogaard K, Bech KT, Mogensen O, Jensen PT. Musculoskeletal pain among surgeons performing minimally invasive surgery: a systematic review. *Surg Endosc* 2017;31:516–26.
- [7] Yohannes P, Rotariu P, Pinto P, Smith AD, Lee BR. Comparison of robotic versus laparoscopic skills: is there a difference in the learning curve? *Urology* 2002;60:39–45.
- [8] Heemskerk J, Bouvy ND, Baeten CGMI. The end of robot-assisted laparoscopy? A critical appraisal of scientific evidence on the use of robot-assisted laparoscopic surgery. *Surg Endosc* 2014;28:1388–98.
- [9] Tonet O, Focacci F, Piccigallo M, Cavallo F, Uematsu M, Megali G, et al. Comparison of control modes of a hand-held robot for laparoscopic surgery. In: Larsen R, Nielsen M, Sporning J, editors. *Medical Image Computing and Computer-Assisted Intervention—(MICCAI)*. Springer; 2006. p. 429–36.
- [10] Piccigallo M, Focacci F, Tonet O, Megali G, Quaglia C, Dario P. Hand-held robotic instrument for dextrous laparoscopic interventions. *Int J Med Robot* 2008;4:331–8.